

DEPARTMENT OF THE ARMY TECHNICAL BULLETIN

CALIBRATION PROCEDURE FOR INTERMEDIATE FREQUENCY TEST SET AN/GRM-63 (NSN 6625-00-089-4653)

Headquarters, Department of the Army, Washington, DC
29 August 1975

	Paragraph	Page
Section I. INTRODUCTION AND DESCRIPTION		
Purpose and Scope	1	1
Reporting of technical bulletin improvements .	2	2
Description	3	3
General Instructions .	4	3
Differences among models	5	3
II. EQUIPMENT REQUIREMENTS		
Equipment required	6	3
Accessories required .	7	3
III. CALIBRATION PROCESS		
Preliminary procedure	8	4
First IF amplifier/second IF simulator response . .	9	4
Modulator detector alignment	10	6
Afc simulator test	11	7
Afc error indicator	12	7
Signal level meter calibration	13	8
Discriminator meter calibration	14	9
Power supply AC output voltage measurements	15	10
Power supply DC output voltage measurements	16	10
Final procedure	17	11


Section I. INTRODUCTION AND DESCRIPTION

1. Purpose and Scope. a. This bulletin provides **information** for the periodic calibration of Intermediate Frequency Test Set, AN/GRM-63 (fig. 1) which is used by calibration personnel. Since calibration personnel are trained and qualified in the use of calibration test and measuring equipment, detailed instructions concerning the operation and

use of the standards are not contained in this bulletin.

b. This bulletin contains illustrations that locate all controls and components used in the calibration procedure as well as diagrams showing equipment setups. Equipment ground connections are not necessarily shown in the diagrams.

*This bulletin supersedes TB 11-6625-657-35/1, 29 April 1968.

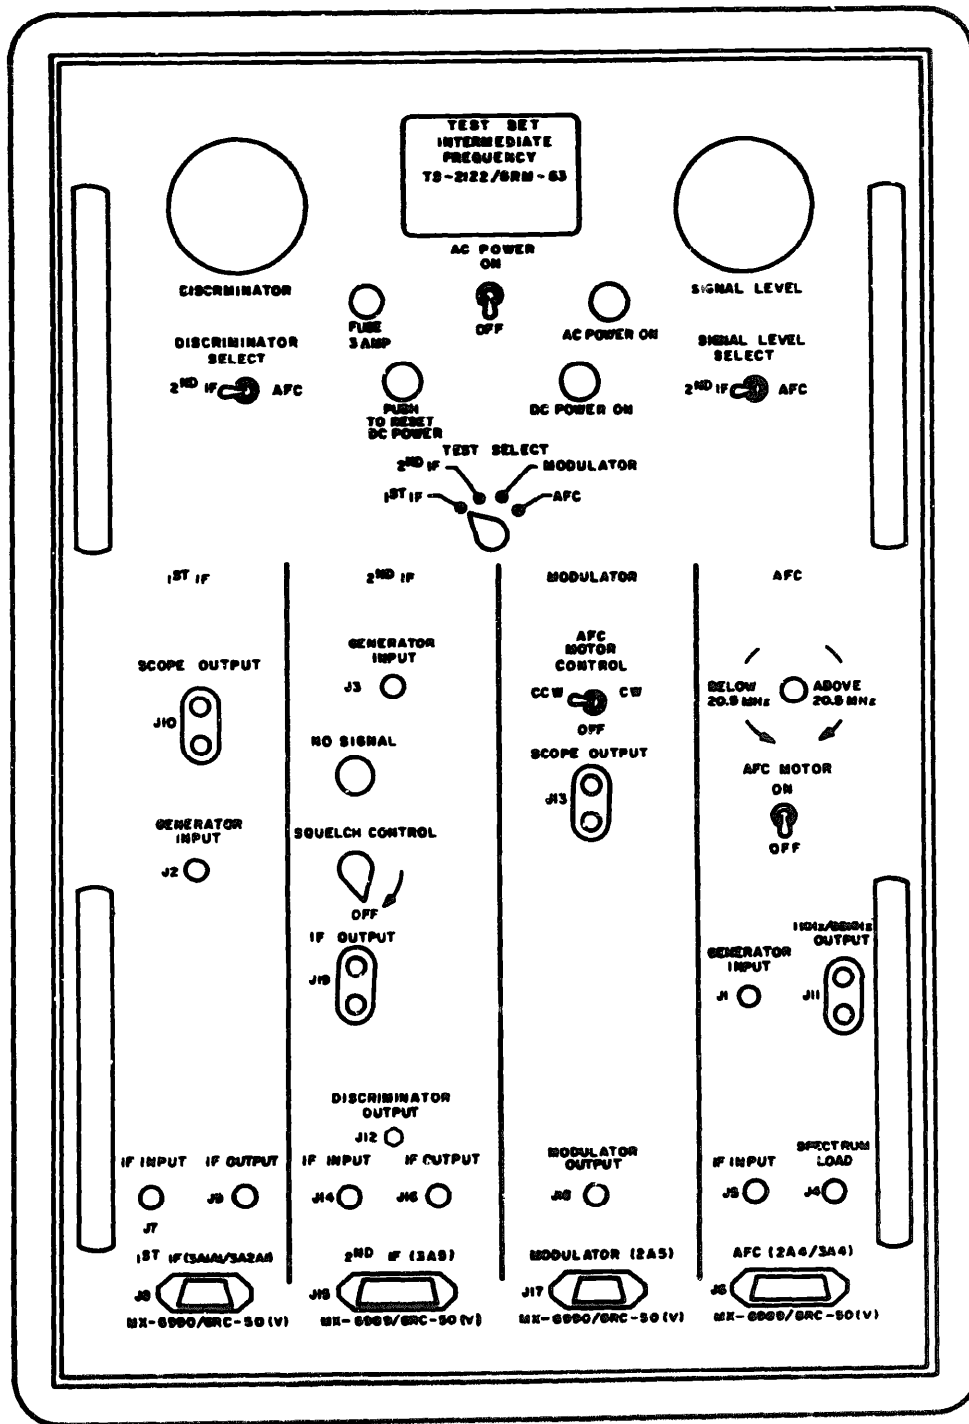

EL6625-657-35-YB-1

Figure 1. Test Instrument, front panel view